

# Journal of Biomedical Optics

BiomedicalOptics.SPIEDigitalLibrary.org

## **Sensing, monitoring, and release of therapeutics: the translational journey of next generation bandages (Erratum)**

Zongxi Li  
Haley Marks  
Conor L Evans  
Gabriela Apiou-Sbirlea

**SPIE.**

Zongxi Li, Haley Marks, Conor L Evans, Gabriela Apiou-Sbirlea, "Sensing, monitoring, and release of therapeutics: the translational journey of next generation bandages (Erratum)," *J. Biomed. Opt.* 24(2), 029802 (2019), doi: 10.1117/1.JBO.24.2.029802.

# Sensing, monitoring, and release of therapeutics: the translational journey of next generation bandages (Erratum)

Zongxi Li,<sup>a</sup> Haley Marks,<sup>b</sup> Conor L Evans,<sup>b</sup> and Gabriela Apiou-Sbirlea<sup>a,b</sup>


<sup>a</sup>Mass General Research Institute, Boston, Massachusetts, United States

<sup>b</sup>Massachusetts General Hospital, Harvard Medical School, Wellman Center for Photomedicine, Charlestown, Massachusetts, United States

[DOI: [10.1117/1.JBO.24.2.029802](https://doi.org/10.1117/1.JBO.24.2.029802)]

This article [*J. Biomed. Opt.* **24**(2), 021201 (2019), doi: [10.1117/1.JBO.24.2.021201](https://doi.org/10.1117/1.JBO.24.2.021201)] was originally published online on 27 December 2018 with an error in Fig. 2. The four references cited in the bottom half of Fig. 2 should be 8, 22, 19, and 20, instead of 8, 14, 11, and 12.

The corrected figure, printed here below, includes those reference citations.

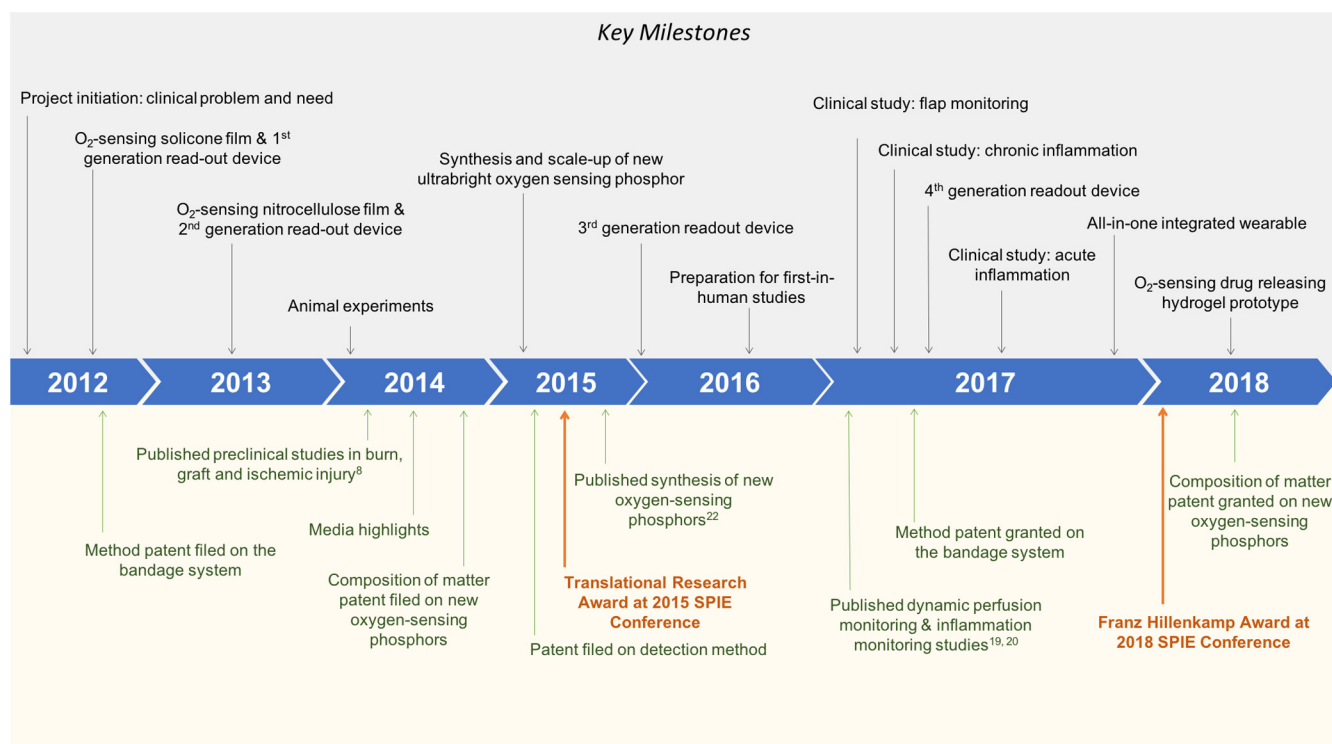

**Fig. 2** Key milestones throughout the oxygen-sensing SMART bandage translational journey. The top half of Fig. 2 summarizes the thirteen milestones, while the bottom half of the figure shows the most relevant publications, new intellectual property, and awards

The correct references for the figure are as follows:

8. Z. Li et al., "Non-invasive transdermal two-dimensional mapping of cutaneous oxygenation with a rapid-drying liquid bandage," *Biomed. Opt. Exp.* **5**(11), 3748–3764 (2014).
19. P. G. L. Koolen et al., "Oxygen-sensing paint-on bandage: calibration of a novel approach in tissue

perfusion assessment," *Plast Reconstr. Surg.* **140**(1), 89–96 (2017).

20. Z. Li et al., "Non-invasive monitoring of skin inflammation using an oxygen-sensing paint-on bandage," *Biomed. Opt. Express* **8**(10), 4640–4651 (2017).
22. E. Roussakis et al., "'Clickable' porphyrins for the visualization of oxygenation under ambient light," *Angew. Chem. Int. Ed.* **54**(49), 14728–14731 (2015).

This article was corrected online on 18 January 2019. It appears correctly in the print issue of *J. Biomed. Opt.* **24**(2).