

Journal of Medical Imaging

MedicalImaging.SPIEDigitalLibrary.org

Back-irradiated and dual-screen sandwich detector configurations for radiography (Erratum)

Anthony R. Lubinsky
Adrian Howansky
Hao Zheng
Wei Zhao

Back-irradiated and dual-screen sandwich detector configurations for radiography (Erratum)

Anthony R. Lubinsky, Adrian Howansky, Hao Zheng, and Wei Zhao
 Stony Brook University, Department of Radiology, Health Sciences Center, Stony Brook, New York, United States

[DOI: [10.1117/1.JMI.6.3.039801](https://doi.org/10.1117/1.JMI.6.3.039801)]

This article [*J. Med. Imag.* 6(3), 033501 (2019), doi: [10.1117/1.JMI.6.3.033501](https://doi.org/10.1117/1.JMI.6.3.033501)] was originally published online on 9 July 2019. In the original version of the article, there was a clerical error in the construction of the curves in Fig. 3(b) from a matrix of calculated results. This has no effect on the conclusions of the article. The original figure and the corrected figure are provided here (the caption did not change).

Original:

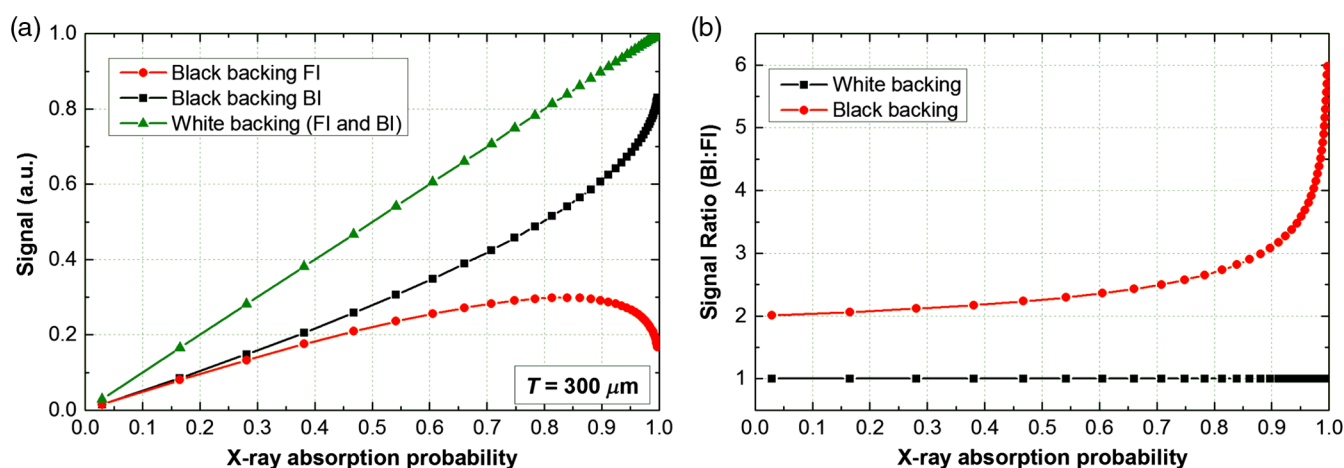


Fig. 3 Comparison of (a) DC signal for a single screen ($T = 300 \mu\text{m}$) with white or black backing, in FI and BI, for a given exposure. (b) The corresponding ratio of BI:FI signal.

Corrected:

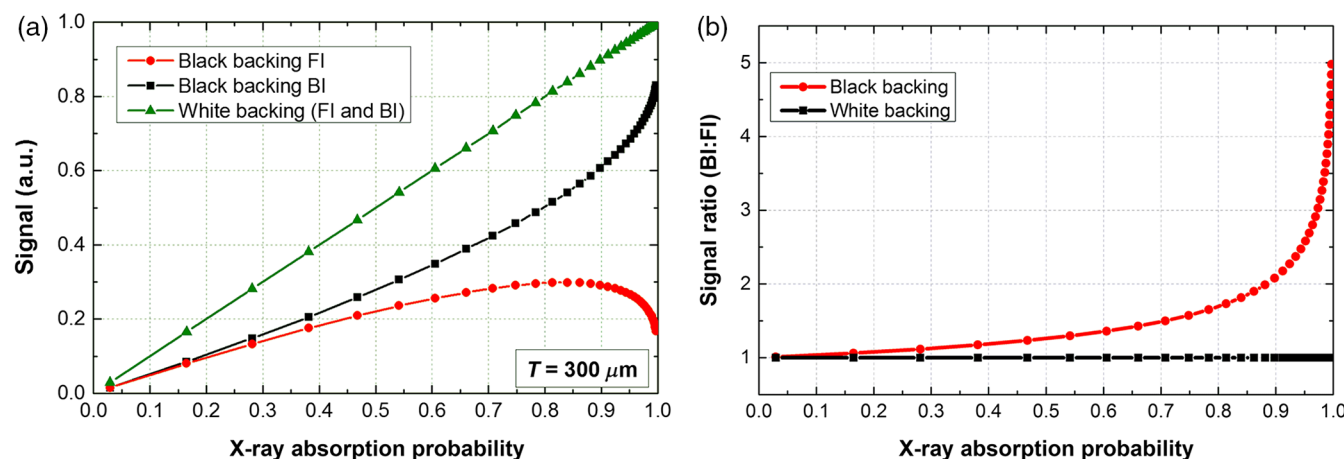


Fig. 3 Comparison of (a) DC signal for a single screen ($T = 300 \mu\text{m}$) with white or black backing, in FI and BI, for a given exposure. (b) The corresponding ratio of BI:FI signal.

This article was corrected online on 25 July 2019. It appears correctly in print.